

YAGI et al Q66253 OXYGEN ENRICHING APPARATUS,... Filed: September 21, 2001 Abraham J. Rosner 202-293-7060 1 of 6

[DOCUMENT NAME]


[FIG. 1]

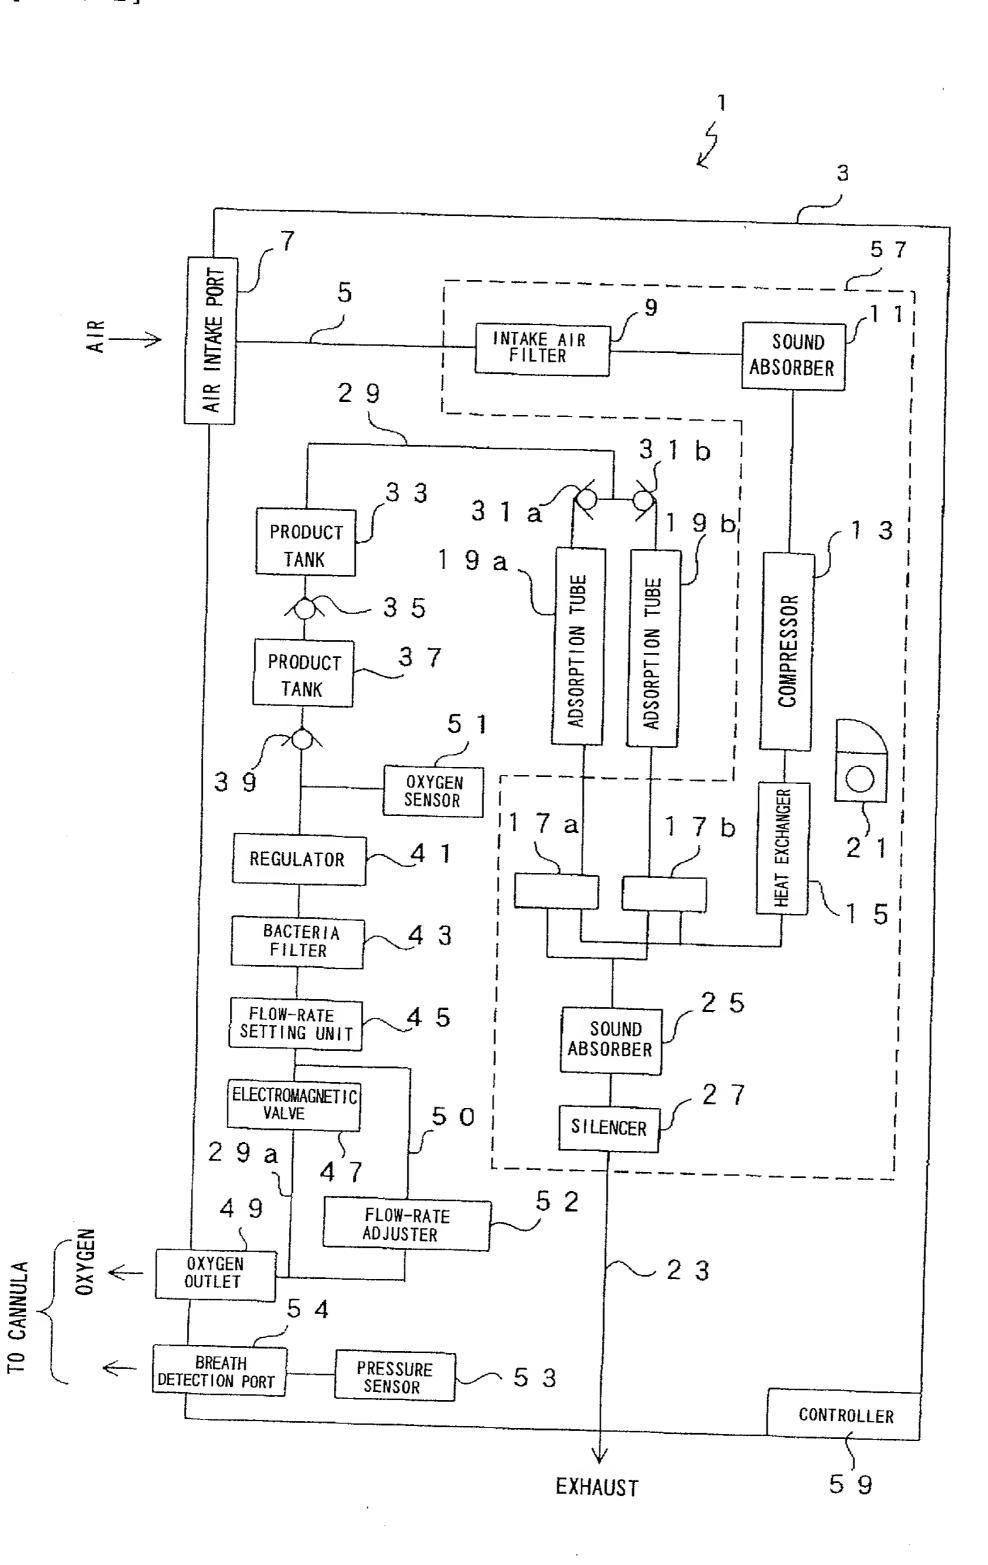

[FIG. 2]

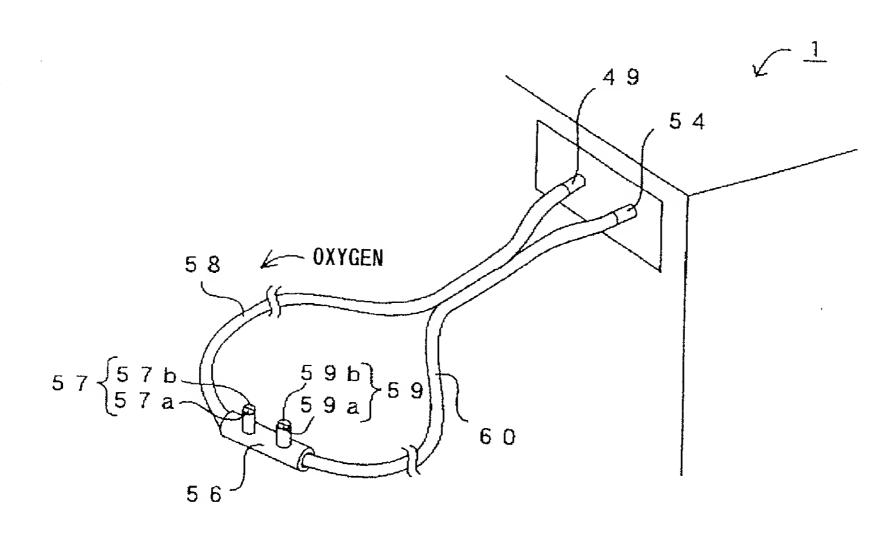

[FIG. 3]

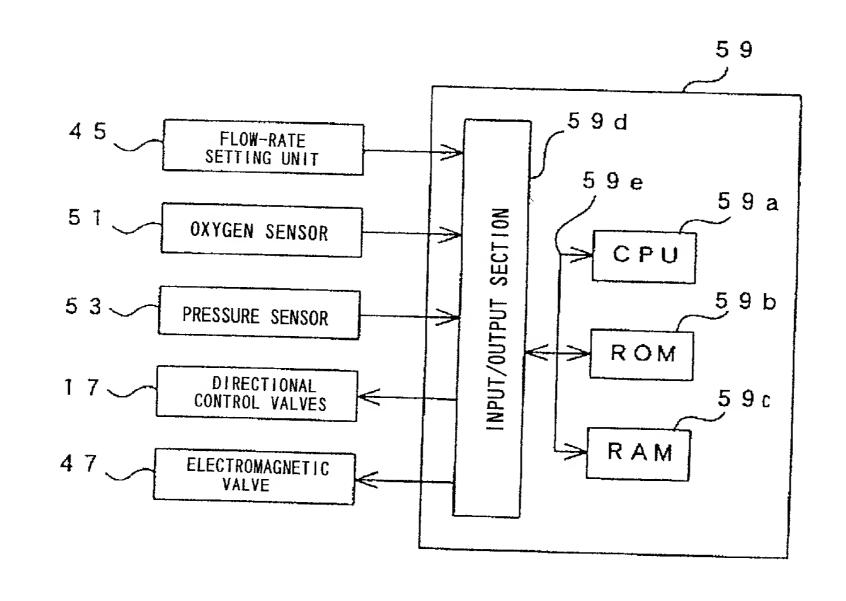


And the state of t

YAGI et al Q66253 OXYGEN ENRICHING APPARATUS,... Filed: September 21, 2001 Abraham J. Rosner 202-293-7060 3 of 6

[FIG. 4]


BREATHING CYCLE PATTERN MODEL

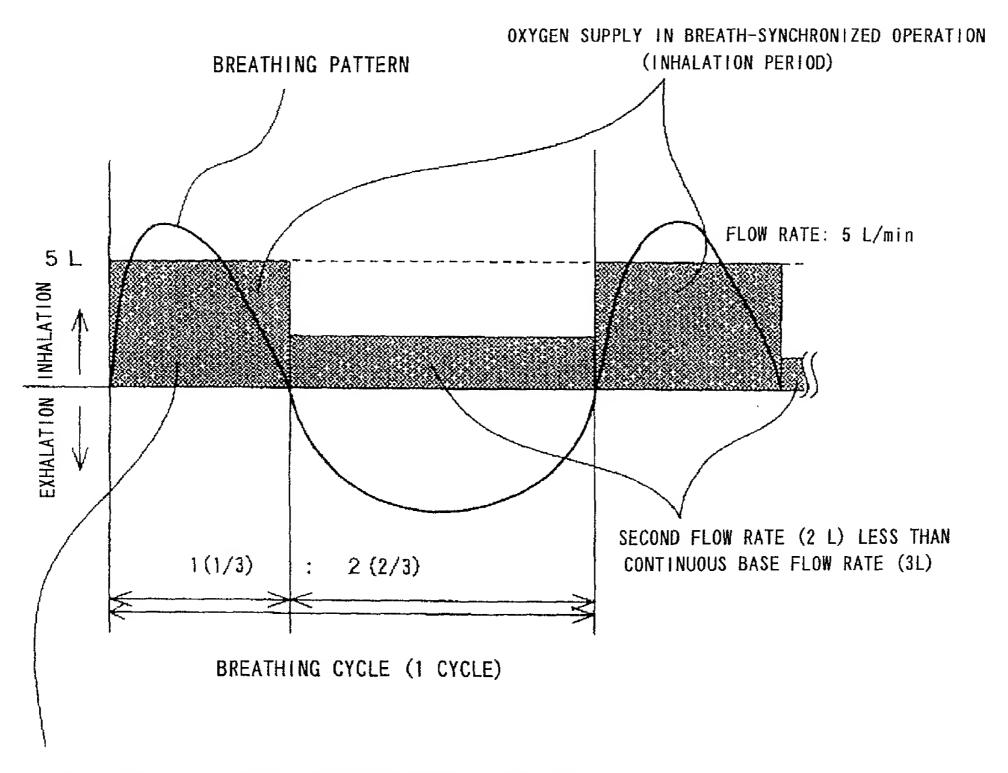

FLOW OF OXYGEN WHEN BREATH SYNCHRONIZATION IS EFFECTED (SET FLOW RATE: 5 L)


YAGI et al Q66253 OXYGEN ENRICHING APPARATUS,... Filed: September 21, 2001 Abraham J. Rosner 202-293-7060 4 of 6

[FIG. 5]

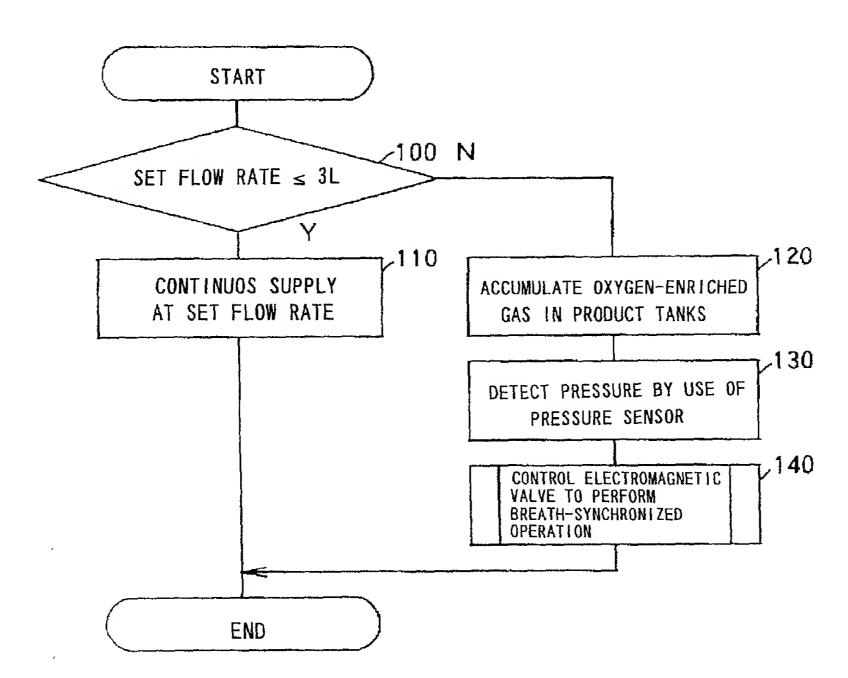


YAGI et al Q66253 OXYGEN ENRICHING APPARATUS,... Filed: September 21, 2001 Abraham J. Rosner 202-293-7060 5 of 6

[FIG. 6]

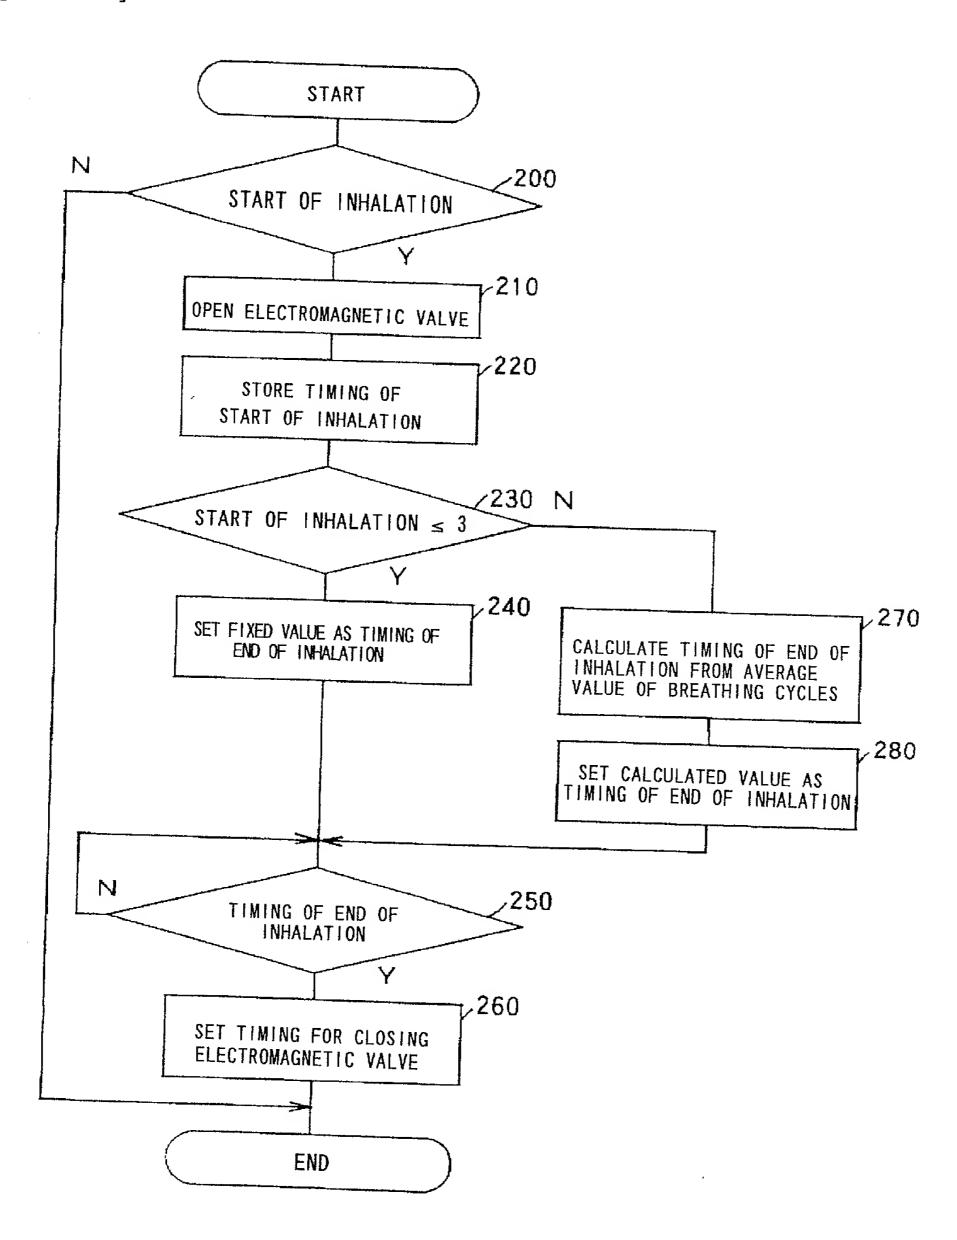

[FIG. 7]

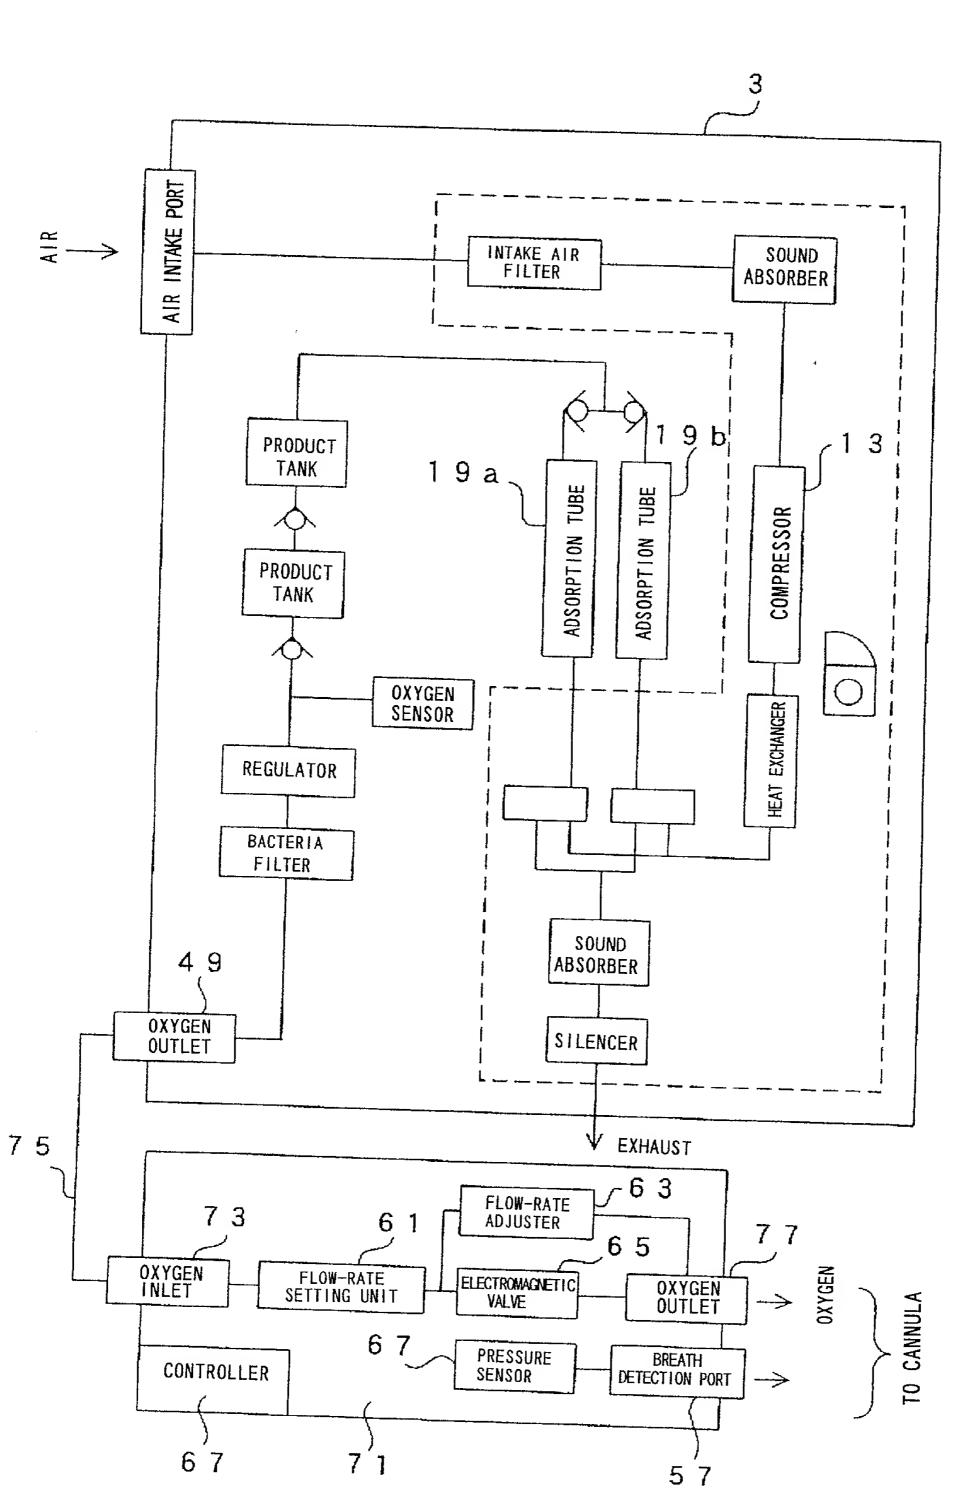

ping profit spots there also also being pasts and also being pasts and also being pasts and also being the pasts and a past a past and a past and a past a past and a past a